## Republic of the Philippines

City of San Carlos

Negros Occidental

#### SHEET NO. 1

### INVITATION TO BID

## PURCHASE REQUEST NO: 1-25-06-0952


Sealed bids for quotation of prices will be received for the purchase of the following supplies, materials and equipment of the government to be opened on the date, place and time stated in INSTRUCTION TO BIDDERS.

ITEM #	QTY.	UNIT	ARTICLES	U PRICE	TOTAL
1	1		Delivery Term: 30 Calendar Days upon receip AUTOCLAVE MACHINE FEATURES: Sterilizing course: Automatic sterilization controlled computer, easy to operate Specifications: Sterilizing Chamber Volume: $16L - 18L$ Working pressure: $0.21Mpa - 0.23Mpa$ Working Temperature: $130^{\circ}C - 134^{\circ}C$ , Suitable for 4-6minutes of fla Temperature Adjust Range: $105^{\circ}C - 134^{\circ}C$ Time Range: $0 - 60$ min Heat Average: $\leq \pm 1^{\circ}C$ Power: $1.2KW - 1.5KW/AC$ , $220V$ , $49HZ$ -50HZ Sterilizing Plate (mm): $335mm - 340mm \times 190mm$ - $200mm$ 3 - 4 pieces plate Dimension (mm): $540mm - 545mm \times 325mm$ - $330mm = 540mm - 620mm \times 400mm - 410mm$ Net Weight : $14kg - 16kg$ Gross Weight: $16kg - 18kg$	by ash sterilizing x 25mm-30mm x 420mm - 425mm	
F	PURPOSE		X-X-X-X-X-X-X-X-X-X-X-X-X-X-X-X-X-X-X-	cy TOTAL ncy =	

Name / Signature of Representatives

Form & Amount of Bid Security

# **INSTRUCTION TO BIDDERS**

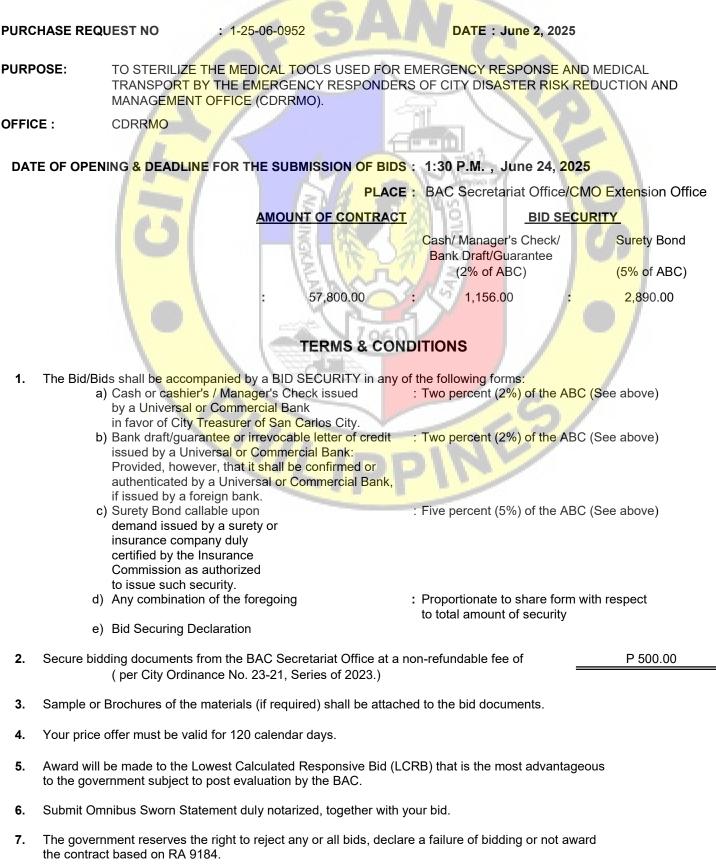

8. Electronic submission and receipt of bids is not available pending compliance with GPPB Resolutions.

SGD ATTY. MA. CHAT H. DELIMA-CORDERO City Gov't Dept. Head I-OHRM / BAC Chairman BIDS & AWARDS COMMITTEE